Biomedical Optics

SPIEDigitalLibrary.org/jbo

Least squares QR-based decomposition provides an efficient way of computing optimal regularization parameter in photoacoustic tomography

Calvin B. Shaw Jaya Prakash Manojit Pramanik Phaneendra K. Yalavarthy



Least squares QR-based decomposition provides an efficient way of computing optimal regularization parameter in photoacoustic tomography

Calvin B. Shaw,^a Jaya Prakash,^a Manojit Pramanik,^b and Phaneendra K. Yalavarthy^a

^aSupercomputer Education and Research Centre, Indian Institute of Science, Bangalore 560012, India

^bDepartment of Electrical Engineering, Indian Institute of Science, Bangalore 560012, India

Abstract. A computationally efficient approach that computes the optimal regularization parameter for the Tikhonov-minimization scheme is developed for photoacoustic imaging. This approach is based on the least squares-QR decomposition which is a well-known dimensionality reduction technique for a large system of equations. It is shown that the proposed framework is effective in terms of quantitative and qualitative reconstructions of initial pressure distribution enabled via finding an optimal regularization parameter. The computational efficiency and performance of the proposed method are shown using a test case of numerical blood vessel phantom, where the initial pressure is exactly known for quantitative comparison. © 2013 Society of Photo-Optical Instrumentation Engineers (SPIE) [DOI: 10.1117/1.JBO.18.8.080501]

Keywords: photoacoustic tomography; image reconstruction; regularization.

Paper 130412LR received Jun. 14, 2013; revised manuscript received Jul. 4, 2013; accepted for publication Jul. 9, 2013; published online Jul. 31, 2013.

Photoacoustic (PA) imaging is an emerging, noninvasive, *in vivo* biomedical imaging modality.^{1,2} A nanosecond laser pulse is generally used to irradiate biological tissue, resulting in a temperature rise from optical absorption and subsequently producing pressure waves due to thermoelastic expansion.² The pressure waves are then acquired using a wide-band ultrasonic transducer at various locations around the surface of the tissue. A reconstruction algorithm is deployed that maps the initial pressure rise (proportional to the absorbed optical energy density) within the tissue from the recorded PA signals.³

Several PA image reconstruction algorithms were proposed in the literature, ^{4,5} including analytical algorithms in the form of

Address all correspondence to: Manojit Pramanik, Department of Electrical Engineering, Indian Institute of Science, Bangalore 560012, India. Tel: (+91) 80 2372; Fax: (+91) 80 2360 0444; E-mail: manojit@ee.iisc.ernet.in or Phaneendra K. Yalavarthy, Supercomputer Education and Research Centre, Indian Institute of Science, Bangalore 560012, India. Tel: (+91) 80 2293 2496; Fax: (+91) 80 2360 2648; E-mail: phani@serc.iisc.in

filtered back projection (BP) or algorithm based on Fourier transform. Their limitations include the requirement of large amount of data and are limited in terms of quantitative estimation. To overcome this limitation, various iterative image reconstruction algorithms have been proposed to improve the quantative accuracy of the reconstructed images, at the same time being computationally efficient. Moreover, in case of full-view data sets, the least squares QR (LSQR)-based reconstruction scheme was used, which indirectly provides regularized solution with an added advantage of being highly efficient. The limited-view data is reconstructed using a standard Tikhonov regularization, which is time consuming and requires an explicit regularization parameter. 5–8

In this letter, we propose a Tikhonov regularization framework based on LSQR decomposition, where Q and R represent an orthogonal and upper triangular matrices, respectively, which uses Lanczos bidiagonalization to provide dimensionality reduction to the system of equations in the case of limited-view data set. This is further used to carry out a simplex method-based optimization procedure to find the optimal regularization parameter. The performance of the proposed method is compared with the generalized cross validation (GCV)⁹ and L-curve⁹ methods, along with the analytical methods, such as BP⁴ and k-wave-based time-reversal reconstruction¹⁰ using a numerical blood vessel network phantom.

The system matrix approach has been adopted here to describe the PA data collection process, which can be represented by a Toeplitz matrix of a time-varying causal system. The image (dimension of $n \times n$) is converted into a long vector by stacking all columns one below the other, represented by x(dimension of $n^2 \times 1$). The system matrix (A) has a dimension of $m \times n^2$. Here, each column of **A** represents the impulse response corresponding to each pixel in the image. Moreover, the time-varying data is stacked to result in a long vector having dimensions $m \times 1$ (which makes the number of rows of A to be m). In order to improve the computation time for building the system matrix, the system response was measured only once for the corner pixel [making x(corner pixel) = 1 and the rest of the entries were made zero], which forms the first column entry of A. The rest of the columns $(n^2 - 1)$ are filled by using shifting and attenuation properties of the PA signal. This approach assumes that the medium has homogeneous ultrasound properties.

The system response for the corner pixel is recorded using k-wave MATLAB toolbox, 10 which simulates the PA wave prorogation in two dimension. The simulation geometry had a computational grid of 701×701 pixels (0.1 mm/pixel). Forty detectors were placed in a circular fashion of 34-mm radius. Each detector was assumed to be a point detector with a frequency response of 2.25 MHz as center frequency and 70% bandwidth. The imaging region was restricted to 201×201 pixels located at the center, resulting in $n^2 = 40,401$. A time step of 50 ns having 1000 time steps was used in recording each signal (making m = 40,000). The simulations assumed a sound speed of 1500 m/s.

In summary, the forward model of PA imaging can be written as

$$\mathbf{A}x = b,\tag{1}$$

0091-3286/2013/\$25.00 © 2013 SPIE

where x is a long column vector (unknown, representing the initial pressure rise, p_0) and b is a measurement vector. The simple BP (analytical) image reconstruction scheme becomes⁴

$$x = \mathbf{A}^T b, \tag{2}$$

where *T* represents the transpose of the matrix. As it is noniterative, this method is computationally efficient but known to provide only qualitative results.⁴

Both BP and time-reversal methods are analytical in nature but lack the quantitative nature of the results.⁵ In cases of limited data, typically a model-based reconstruction is employed which relies on minimizing the data-model misfit along with a regularization function, therefore the objective (cost) function in this case can be written as

$$\Omega = \|\mathbf{A}x - b\|_{2}^{2} + \lambda \|x\|_{2}^{2},\tag{3}$$

where λ is the regularization parameter. The ℓ_2 -norm is represented by $\|.\|_2^2$. The function Ω is minimized with respect to x, leading to a direct solution

$$x = (\mathbf{A}^{\mathsf{T}}\mathbf{A} + \lambda \mathbf{I})^{-1}\mathbf{A}^{\mathsf{T}}b. \tag{4}$$

The GCV method⁹ is the most popular automated approach for estimating the optimal regularization parameter λ_{opt} using following function

$$G(\lambda) = \frac{\sum_{i=1}^{\text{rank}(A)} \left(\frac{H_i^T b}{\sigma_i^2 + \lambda^2}\right)^2}{\left(\sum_{i=1}^{\text{rank}(A)} \frac{1}{\sigma_i^2 + \lambda^2}\right)^2},$$
 (5)

where the SVD of $\mathbf{A} = \mathbf{H} \Sigma \mathbf{G}^T$ where, Σ is a diagonal matrix containing singular values (σ) . The left and right orthogonal matrices are given by \mathbf{H} and \mathbf{G} , respectively. The L-curve is another popular scheme for estimating the optimal regularization parameter. The corner of L-curve gives the optimal regularization value, and as with GCV method, it does not require any prior information. The LSQR method is one of the variants of the conjugate gradient method used to solve a large system of equations. One of the main contributions of this letter is to use the LSQR-type algorithm to optimally determine the regularization parameter in PA image reconstruction. This is accomplished by using a Lanczos bidiagonalization of the system matrix (\mathbf{A}). The left and right Lanczos matrices along with the bidiagonal matrix are related to the system matrix as shown below: 11,12

$$U_{k+1}(\beta_0 e_1) = b, \, \mathbf{A}V_k = U_{k+1}B_k, \tag{6}$$

$$\mathbf{A}^T U_{k+1} = V_k B_k^T + \alpha_{k+1} v_{k+1} e_{k+1}^T, \tag{7}$$

where B represents the lower bidiagonal matrix, and U and V represent the left and right orthogonal Lanczos matrices, respectively. The unit vector of dimension $k \times 1$ is represented by e_k (= 1 at the k'th row and 0 elsewhere). Note that the dimensions of U_k and V_k are $(m \times k)$ and $(n^2 \times k)$, with k representing the number of iterations in the bidiagonalization procedure. Finally, u_i and v_i represent the left and right Lanczos vectors. The B_k is the bidiagonal matrix having $\alpha_1, \ldots, \alpha_k$ in the main diagonal

and β_1, \dots, β_k in the lower subdiagonal of the matrix with a dimension of $[(k+1) \times k]$.

Now the Tikhonov minimization update for the equation for the LSQR-type method¹² is given by [which is equivalent to Eq. (4)]:

$$x^{k} = (B_{k}^{T}B_{k} + \lambda I)^{-1}\beta_{0}B_{k}^{T}e_{1}.$$
 (8)

Here β_0 is the ℓ_2 -norm of b. Once, x^k (reduced x) is estimated then the initial pressure can be obtained using the relation $p_0 = x = V_k x^k$.

Determination of the optimal number of Lanczos iterations (k^{opt}) and optimal regularization parameter λ_{opt} is given in Algorithm 1. The advantage of LSQR-type method in finding the initial pressure rise distribution p_0 lies in its dimensionality reduction capability which makes the update as x^k [Eq. (8)] with $k \ll n^2$. The major role in the entire optimization procedure is characterized by k (number of Lanczos bidiagonalization). This factor determines the size of the bidiagonal matrix, B_k [dimension of $(k+1) \times k$. In this work, the optimal number of Lanczos iterations turned out to be 25 obtained using Algorithm 1, making $k^{\text{opt}} = 25$. The optimal λ is searched within the specified bound (λ_{lim}) and is set to 1000. A gradient-free simplex method type algorithm is used due to its computational efficiency to compute the optimal regularization parameter (λ_{opt}) . The λ^{opt} is found corresponding to k=25is chosen for LSQR method. Using these in Eq. (8) gave x^k and subsequently $p_0(x)$.

A Linux workstation with Intel Xeon Dual Quad Core 2.33 GHz processor having 64 GB memory was used in all computations carried out in this work.

In order to show the effectiveness of the proposed method, a numerical blood vessel phantom was chosen. Note that measuring actual p_0 in the experimental phantom case is extremely challenging, which makes the comparison of performance of the methods discussed here difficult. Figure 1(a) shows the blood vessel network used as a numerical phantom with a maximum initial pressure rise of 1 kPa. The k-wave tool box 10 was used to generate the simulated PA data with 40 detectors around the object of interest. Subsequently, the simulated data had a signal-to-noise-ratio of 40 dB (1% noise) to mimic the real

Algorithm 1 Algorithm for determining optimal number of Lanczos iterations and optimal regularization.

- Input: Lanczos Bidiagonal Matrix B_k; V_k (k = 1, 2, ..., 50);
 b; β_Ω; A; λ_{lim}.
- Output: Optimal number of Lanczos iterations: $k^{\rm opt}$ and optimal regularization parameter: $\lambda^{\rm opt}$
- for k = 1, 2, ..., 50 do Steps 1–3
- 1. Estimate the optimal λ for the given $k(\lambda_k^{\text{opt}})$ Simplex method is used to find λ_k^{opt} in the range of [O λ_{lim}], with $x = V_k * x^k$, found using Eq. (8).
- 2. Compute x^k with $\lambda = \lambda_k^{\text{opt}}$ using Eq. (8). $x = V_k x^k$
- 3. Estimate $\operatorname{res}^k = \|b A * x\|_2^2$ $k^{\operatorname{opt}} = \operatorname{index}$ of minimal value of res^k and $\lambda^{\operatorname{opt}} = \lambda_{\operatorname{popt}}^{\operatorname{opt}}$

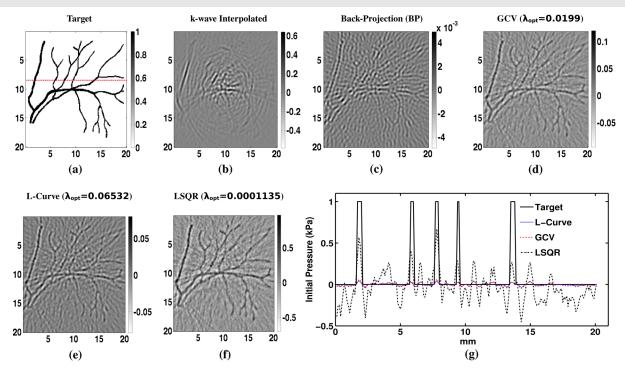


Fig. 1 (a) Numerical blood vessel phantom is used for the study (dimensions are in measured in millimeters). (b–f) Reconstructed photoacoustic images using k-wave interpolated, backprojection, reconstructions using λ [Eq. (4)] obtained by GCV [Eq. (5)], L-curve and LSQR [Eq. (8)] methods, respectively. (g) One-dimensional cross-sectional plot for the results presented in (a),(d),(e), and (f) along the dotted line shown in (a).

experimental situation. The reconstruction results obtained using various methods are shown in Fig. 1(b)-1(f). The proposed method's result is shown in Fig. 1(f), with the value obtained for $\lambda_{\rm opt}$ shown in the parenthesis at the top of the image. Figure 1(g) shows the one-dimensional cross-sectional plot for the reconstructed PA image using GCV, L-curve, and LSQR-based methods as well as target image [along the dotted line in Fig. 1(a)], quantitatively showing an improvement of at least 10 times in the recovered p_0 . As seen from Fig. 1, the performance of LSQR-type method is superior in terms of quantitation compared to their counterparts. The total computational time recorded for all reconstruction methods shown in Fig. 1 are 129.8, 1.3, 7516.5, 7130.7, 444.9 s, respectively (system matrix building time = 181 s). A speed up factor of 17 was achieved by the proposed method compared to GCV method. The results indicate that among the model-based methods, the proposed method (LSQR) is the most efficient and promising technique for real-time imaging.

It is important to note that the LSQR (without explicit regularization) has been extensively used in full-view data cases (where $m \gg n^2$) and shown to be effective in quantitation.⁶⁻⁸ In limited data cases (where $m \ll n^2$), the Tikhonov minimization scheme is more effective with the important condition of finding an optimal regularization parameter. This work addresses this problem of finding an optimal regularization parameter automatically without prior information with an added advantage of reducing the dimensionality of the problem, making it a highly computationally efficient method.

References

- L. H. V. Wang and S. Hu, "Photoacoustic tomography: in vivo imaging from organelles to organs," *Science* 335(6075), 1458–1462 (2012).
- M. Pramanik et al., "Design and evaluation of a novel breast cancer detection system combining both thermoacoustic (TA) and photoacoustic (PA) tomography," *Med. Phys.* 35(6), 2218–2223 (2008).
- J. Gamelin et al., "Curved array photoacoustic tomographic system for small animal imaging," J. Biomed. Opt. 13(2), 024007 (2008).
- G. Paltauf et al., "Iterative reconstruction algorithm for optoacoustic imaging," J. Acoust. Soc. Am. 112(4), 1536–1544 (2002).
- K. Wang et al., "Investigation of iterative image reconstruction in three-dimensional optoacoustic tomography," *Phys. Med. Biol.* 57(17), 5399–5424 (2012).
- X. L. Dean-Ben, V. Ntziachristos, and D. Razansky, "Acceleration of optoacoustic model-based reconstruction using angular image discretization," *IEEE Trans. Med. Imag.* 31(5), 1154–1162 (2012).
- X. L. Dean-Ben et al., "Accurate model-based reconstruction algorithm for three-dimensional optoacoustic tomography," *IEEE Trans. Med. Imag.* 31(10), 1922–1928 (2012).
- A. Buehler et al., "Model-based optoacoustic inversions with incomplete projection data," *Med. Phys.* 38(3), 1694–1704 (2011).
- R. P. K. Jagannath and P. K. Yalavarthy, "Minimal residual method provides optimal regularization parameter for diffuse optical tomography," J. Biomed. Opt. 17(10), 106015 (2012).
- B. E. Treeby and B. T. Cox, "k-Wave: MATLAB toolbox for the simulation and reconstruction of photoacoustic wave fields," *J. Biomed. Opt.* 15(2), 021314 (2010).
- C. C. Paige and M. A. Saunders, "LSQR: An algorithm for sparse linear equations and sparse least squares," ACM Trans. Math. Softw. 8(1), 43–71 (1982).
- J. Prakash and P. K. Yalavarthy, "A LSQR-type method provides a computationally efficient automated optimal choice of regularization parameter in diffuse optical tomography," *Med. Phys.* 40(3), 033101 (2013).