


# Evaluation of standardized performance test methods for biomedical Raman spectroscopy (Erratum)

Andrew M. Fales, Ilko K. Ilev, and T. Joshua Pfefer


U.S. Food and Drug Administration, Center for Devices and Radiological Health, Silver Spring, Maryland, United States

[DOI: [10.1117/1.JBO.27.7.079801](https://doi.org/10.1117/1.JBO.27.7.079801)]

This article [*J. Biomed. Opt.* **27**(7), 074705 (2022) doi: <https://doi.org/10.1117/1.JBO.27.7.074705>] was originally published on 28 October 2022 with an error in Fig. 4. The axes were reversed in the original version:

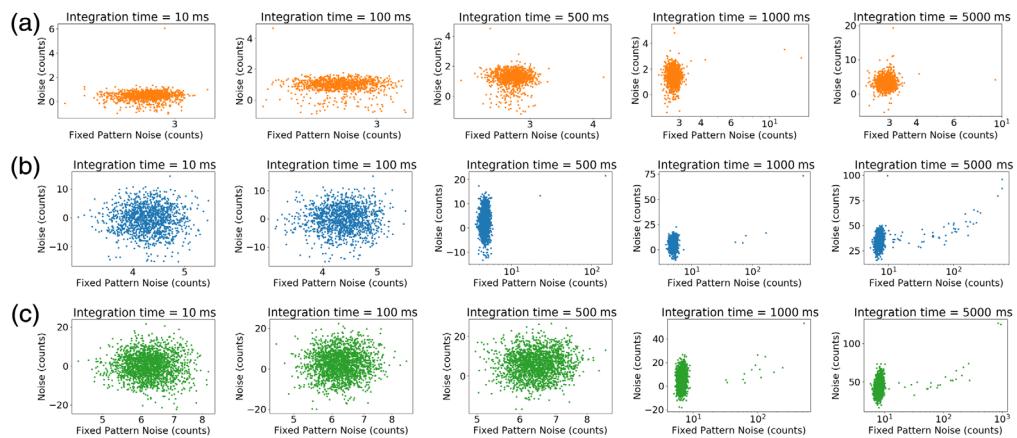

Corrected version:

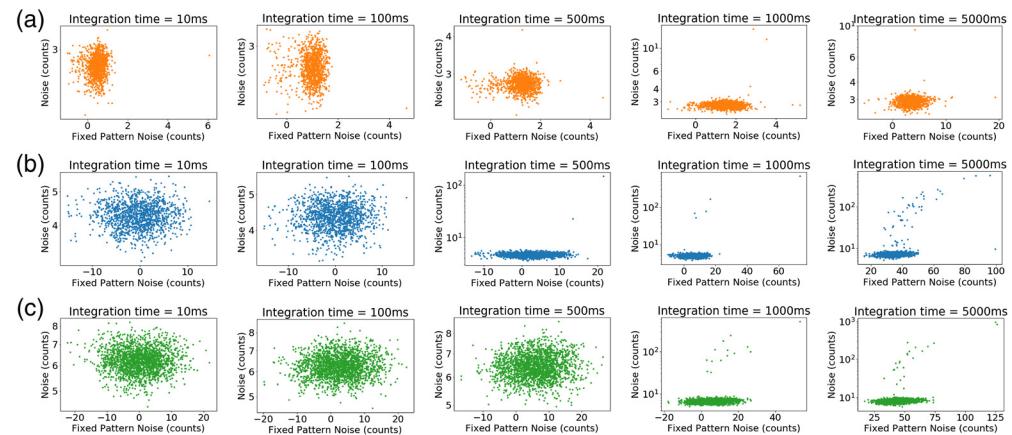

The error was corrected on 9 July 2022.